





CE Europe No. RPS/68/2021-CMC

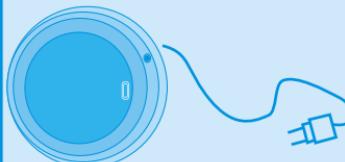



HOW TO USE

READ BEFORE USE

<i>Table of Contents</i>	<i>Page</i>
ABOUT  VACUUM ERECTION SYSTEM	2
DEVICE COMPONENTS	3
MEDICAL INDICATIONS	4
SELECT COMPONENTS FOR YOUR PENIS SIZE	5
GUIDE TO USING THE SYSTEM	6
INSTRUCTIONS FOR ERECTILE DYSFUNCTION THERAPY	8
USING THE DEVICE (STEP BY STEP) - ERECTILE DYSFUNCTION	9
INSTRUCTIONS FOR "SEXUAL FITNESS" THERAPY	10
USING THE DEVICE (STEP BY STEP) - "SEXUAL FITNESS"	11
THE TEST	12
COMMON PROBLEMS AND SOLUTIONS	13
PRECAUTIONS	14-17



Erect-D VACUUM Erection System is a medically-proven high quality penis pump, which is a non-invasive, safe and effective solution to follow a *Sexual Fitness* routine and induce on demand drug-free instant erections as a solution to *Erectile Dysfunction*.

Economically designed and engineered, Erection System consists of a cylinder that fits over the penis, with an electronic motor to create suction and induce a vacuum environment around the penis which draws blood into it and helps the penis to become engorged.


Note:

Charged your **Erect-D** before using (See diagram)


Erect-D Vacuum Pump

On/Off


vacuum release button



On Charging Red light
Full charge Blue light

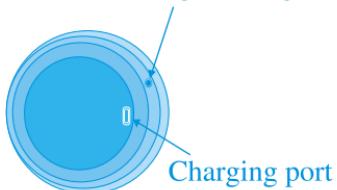


Charging Cable



Note: Read instructions carefully before using **Erect-D**
If instructions are not followed, Erection System will not work.

Adapter: Custom Fitting Adapter Inserts for different penis sizes, to be placed in the penile tube after the ring loading on penile tube then cone is removed.

Put a little amount of lubricant around the base of the penis, the shaft, and glans (see figure).

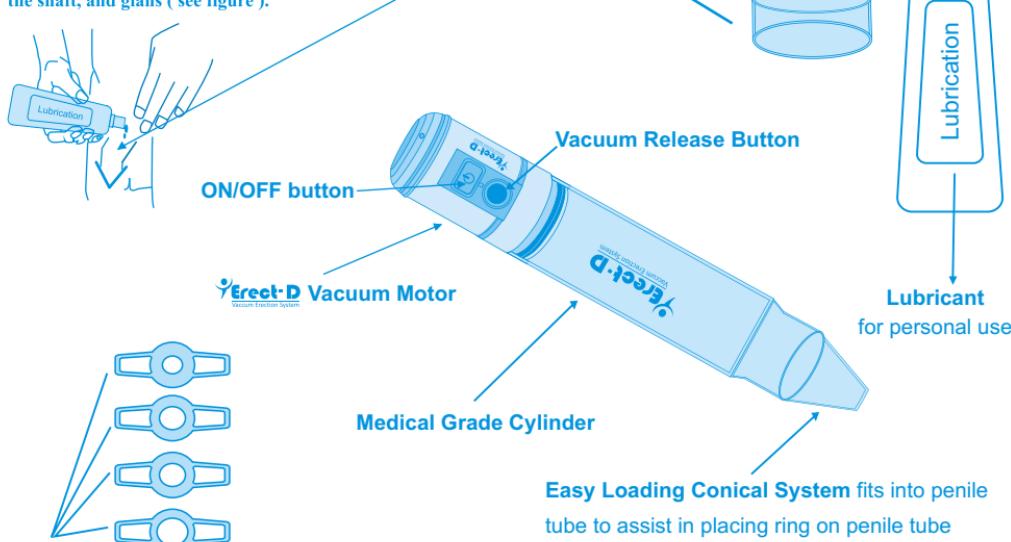

Erect-D Erection Assistant Rings / Constriction Rings:
Vacuum Erection System

to help maintain the erection. For different penile thicknesses

MEDICAL INDICATIONS



ERECTILE DYSFUNCTION

 is meant for the treatment of Erectile Dysfunction. Millions of men are estimated to be affected. Erectile Dysfunction could be a sign of the existence of a serious blood flow or nerve problem. Erectile Dysfunction is often the side effect of a medication you may be taking. If you suspect this, talk to your doctor. You should never change or stop taking medication without first consulting your doctor. Smoking, alcoholism and drug abuse can all contribute to an erectile disorder.

Erectile Dysfunction Therapy with  , recommended for:

Men who sometimes fail to get a full erection due to stress, excitement or fear.

Men who easily get an erection but have problems maintaining it.

Men with erection problems of all ages, even those who haven't achieved an erection in several years.

Men with erection problems who can not take anti-ED drugs due to heart problems.

"SEXUAL FITNESS"

Vacuum environments increase blood flow into the penis when becoming engorged. Over time, regularly induced vacuum environments make the corpus cavernosum adapt to these continuously demanding situations. The penis ends up producing the referred increased blood flow by itself, even when no vacuum environment is created. This implies that the sexual organ reacts faster and stronger to sexual stimulation. A prolonged erection problem can lead to shrinkage of the penile tissues and a reduction in penile circulation (non-use atrophy). Regular use of  will duplicate benefits of nocturnal erections, reversing penis shrinkage, reconditioning penile circulation and promoting a return to good penis health.  can help to stretch tissues back to their normal state within as little as 4 weeks of regular use, combined with an improvement in penile circulation. At the same time, you would be inducing full penile engorgement and promoting good penile health.

Sexual Fitness Therapy with  , recommended to:

Men experiencing weak erections.

Men experiencing progressively weaker erections due to aging process, sedentary lifestyle, alcohol or tobacco consumption as well as high cholesterol or high stress levels.

Men with low levels of testosterone (TDS or hypogonadism) and on hormonal supplementation.

SELECT COMPONENTS FOR YOUR PENIS SIZE AND SET THE DEVICE

1. Start with the largest Erection Assistant and Cushioning Rings. If you are unable to hold the vacuum and the erection with the largest rings, gradually use the next smallest Erection Assistant and Cushioning Ring until you are able to hold the vacuum and the erection.
2. Set the cylinder (with the smooth end up) on a flat surface. Place the Easy Loading Conical System in the penile tube.
3. Lubricate the entire surface of the Easy Loading Conical System with the sealing gel.
4. Grasp the two handles of the Erection Assistant Ring as shown. Place your thumb tips on top of the ring next to the Easy Loading Conical System and pull the ring down. Your thumb tips should glide along the surface of the Easy Loading Conical System. Place the Erection Assistant Ring near the end of the tube for later easy loading onto the base of the penis (do not load the ring onto the tube by pulling the handles, they may tear).



Figure (A)



Figure (B)

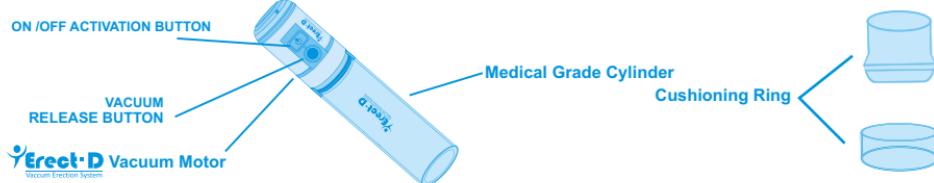


Figure (C)



5. Remove the Easy Loading Conical System and attach the cylinder to the Vacuum Electronic Motor. Twist the cylinder on the motor 1/4 turn, locking it in place. Do not over tighten. Install the Cushioning Rings in the open end of the penile tube.

6. Running warm water over the cylinder (before attaching the motor) will help prevent the cylinder from fogging during use.





ERECTION ASSISTANT RINGS



One of the most important steps is properly fitting the Erection Assistant Rings. To keep blood in the penis, the ring must fit comfortably tight, but should be no tighter than necessary. If **Erect-D** is giving you a good erection but with the Erection Assistant Ring is becoming loose while wearing it in five minutes or less, you need to try the next smaller ring.

Thirty minutes is the maximum recommended time period for wearing the Erection Assistant Rings. If worn longer, permanent damage is possible.

After the correct size ring has been decided, it will only take a few minutes to get an erection.

DO NOT WEAR AN ASSISTANT RING MORE THAN 30 MINUTES.

Erect-D will assist you in reaching a full and satisfying erection in most cases.

Allow a minimum of 30 minutes between uses.

Do not fall asleep wearing the Erection Assistant Ring.

Erection Assistant Rings should not be used as a birth control method.

Use the largest Erection Assistant Ring which holds an erection.

Do not use Erection Assistant Rings while using alcohol or drugs.

Frequent use of Erection Assistant Rings may result in bruising at the base of the penis (where the shaft of the penis meets the pubic area). Temporary side effects may include some bruising of the penis or some small red spots below the skin. Use caution and plenty of water soluble lubricating jelly when removing the support ring.

Do not use oil based lubricants such as petroleum jelly, as they will be harmful to the Erection Assistant Rings and other latex type material such as condoms. Only use water soluble lubricating and sealing gel.

GUIDE TO USING THE SYSTEM

MANUAL VACUUM RELEASE BUTTON AND VACUUM ENVIRONMENT CREATION

Your penis should become filled and rigid without pain in **10 to 90 seconds**. You may feel pressure when your penis starts to become erect from the vacuum, which is normal. If you feel a slight pain when your penis becomes filled, try a lower **vacuum level** by pushing the manual vacuum release button (with a little practice you should find your correct vacuum level, so that you can create a full erection).


The **manual vacuum release button** can be pushed to lower the vacuum level. If too much vacuum is released, it can be easily increased by depressing the activation button.

To **remove the penis from the Cylinder**, push the manual vacuum release button until the vacuum pressure is gone. You can then remove the Cylinder.

Most men with Erectile Dysfunction will lose most of their erection soon after removing their penis from the Cyl-inder. This problem can be solved by correctly fitting the **Erection Assistant Ring**. On the other hand, if you find that you are keeping enough of an erection for intercourse, you may not need to use the **Erection Assistant Ring**. You may be able to have a good sex life while only using the **AED Vacuum** device without the Erection Assistant Rings.

REMOVING THE ERECTION ASSISTANT RING

Caution: Do not wear the Erection Assistant Ring for more than 30 minutes.



Remove the ring by pulling the side loops outwards. The ring will stretch, allowing blood to move from the penis. You can then pull the Erection Assistant Ring off easily. To prevent tangling the Erection Assistant Ring in the pubic hair, try a little sealing gel in the hair before putting on the ring.

1. Lubricate your penis, the inside of the cylinder and pubic hair area (the area that comes in contact with the cushioning rings), with the sealing gel. This helps form a good vacuum seal at your body and prevents the penis from sticking to the walls of the cylinder.
2. Insert the penis into the cylinder and start the vacuum process. Operate the motor by depressing the activation button. Depress the button for approximately 10 seconds, that should create a seal between the system and your body. Continue pressing the button until you have developed a sufficient vacuum. Use the least amount of vacuum necessary to obtain an erection.
3. As soon as the desired erection is achieved, transfer the Erection Assistant Ring from the cylinder onto the base of the penis with your fingertips. Make sure the Erection Assistant Ring is transferred all the way around. Any vacuum that is left can be released by depressing the manual vacuum release button. Practice a few times without the Erection Assistant Ring.

Note 1. After you have been using the system for 30 to 60 days, you may want to recheck the sizing of the rings to be used. For example, you may find that you are now able to use the next size larger rings. Using the larger ring may increase comfort.

Note 2. Some couples may prefer to stop intercourse at least once and reuse the AED Vacuum.


Note 3. If a condom is desired it should be applied after an erection is formed.

Note 4. Following use, the Erection Assistant Ring, the Cushioning Ring and Cylinder can be washed with soap and water, dried and stored. Make sure the Erection Assistant Ring bag is air free and tightly sealed for longer life. DO NOT EVER PUT THE MOTOR IN WATER.


ATTENTION

When placing the Cylinder on the pump head, DO NOT OVER TIGHTEN. Twist one quarter (1/4) turn to tighten. Twisting too hard or too far will break your system. If this happens it WILL NOT be covered under warranty!

USING THE DEVICE (STEP BY STEP) - ERECTILE DYSFUNCTION

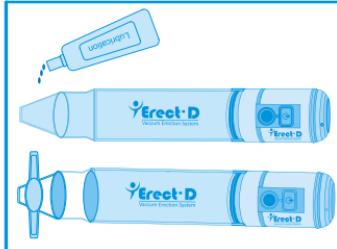


Slide the Erection Assistant Ring over the Easy Loading Conical System and onto the end of the Cylinder. Also lubricant on top of the ring Loading Cone loading.

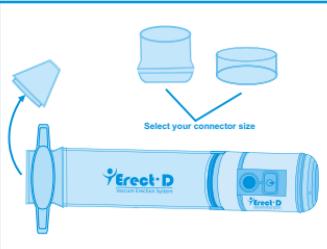


Remove the Easy Loading Conical System and load the Connector Rings.




Lubricate your penis, and your pubic hair area and inside of the Cylinder.
see diagram.

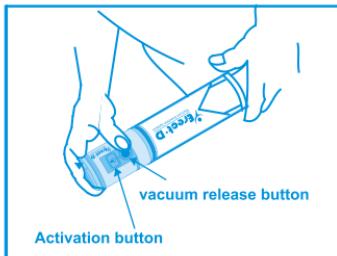

Insert your penis into the prepared Cylinder. if you feel any pain press vacuum release button immediately the pain will disappear.

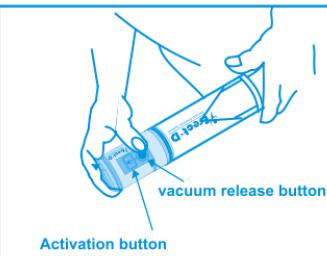

Start the vacuum process with activation button. Once erection is complete slide the ring on to base of the penis once ring transfer is complete. you are ready

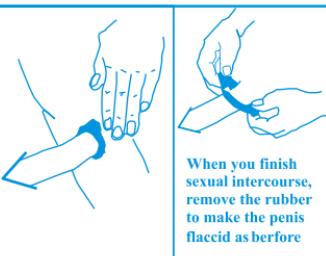


Remove the device by pressing push release vacuum button. When you finish intercourse remove the ring to make the penis flaccid as before.


Instructions for “Sexual Fitness” therapy

Follow steps 1 and 2 as described on page 8.

The therapeutic use of  once a day, from 5 to 7 times per week, may help to maintain penile length, dilate arteries and oxygenate penile tissues. Regular use of  can promote full erectile function. To get started, the components you need to use are:

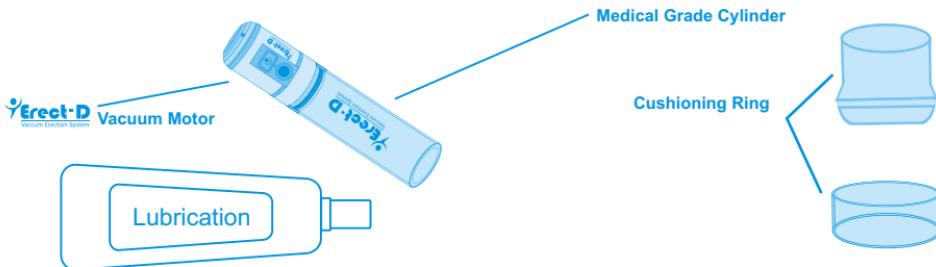

You do not need to use the Erection Assistant Rings. They are designed to hold the blood and maintain an erection that stays rigid during sexual activity. Such rigidity is not necessary for Sexual Fitness Therapy.




Erection Assistant Rings

During a session of Sexual Fitness Therapy we recommend you should aim to produce 5 erections or use  for at least 5-10 minutes. Never operate the motor to the point of causing pain.


USING THE DEVICE (STEP BY STEP) - "SEXUAL FITNESS"



Apply the Sealing Gel on the edge of the Vacuum Cylinder and on the entire length of the penis.

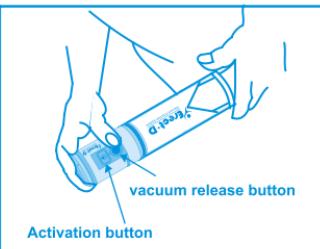

Insert the penis into the

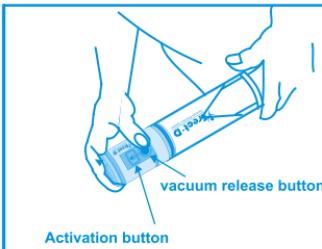

Operate the motor for 10 seconds and then stop for 5 to 10 seconds to slowly create a vacuum environment. Repeat until you gain a full erection.



When you have reached a full erection, wait 30 seconds prior to releasing the vacuum. Tightness and some pressure is normal and expected.



After 30 seconds, release the pressure within the Cylinder by pushing the blue button.



Wait until the penis has returned to a flaccid state and repeat the start-and-stop process again until bringing the penis back to a full erection.

You can make an initial and intuitive assessment of your testosterone level just by answering the following questions:

1. Do you have a decrease in libido (sex drive)? yes no
2. Do you have a lack of energy? yes no
3. Do you have a decrease in strength and endurance? yes no
4. Have you lost height? yes no
5. Have you noticed a decreased "enjoyment of life"? yes no
6. Are you sad and/or grumpy? yes no
7. Are your erections weaker? yes no
8. Have you noticed a recent deterioration in your ability to play sports? yes no
9. Are you falling asleep after dinner? yes no
10. Has there been a recent deterioration in your work performance? yes no

If you have answered "No" to all questions, you are not likely to need further tests.

If you have answered "Yes" to question 1 or question 7, or at least three of the other questions, you may have low testosterone levels and should speak to your doctor or nurse about checking them.

COMMON PROBLEMS AND SOLUTIONS

PROBLEM	LIKELY CAUSE	REMEDY	COMMENTS
No erection	No vacuum because of air leak caused by poor seal	Use more sealing gel; apply firm pressure to body; trim pubic hair; check system for air leaks	Problem is most often associated with inexperience; it stops as you become better at using the system
Partial erection	Not enough practice sessions	More practice using system	Problem most often improves with continued use of system
Rapid Loss of erection (in less than 5 minutes)	Vacuum lost because of air leak, poor seal, poor lubrication	Same as for "No erection". Use smaller or double support rings; remove support ring carefully.	Require that you experiment with varying sizes support rings; see your doctor if you need help or support to continue
Pulling of the skin of the Scrotum	Sealing gel on scrotum; improper pumping technique; inexperience with system	Remove sealing gel from scrotum; continue with practice sessions; angle cylinder downward during pumping	Problem may disappear as you become better at using the system
Discomfort or pain during Pumping	Too rapid pumping; pulling of scrotal tissue	Slower pumping; continue to use the system	Problem usually stops as you become better at using the system
From Erection Assistant Ring	Erection Assistant Ring too small; anxiety	Use larger Erection Assistant Ring; continue to use the system	Problem usually stops as you continue to use the system
During intercourse	Poor lubrication; pressure on a sensitive area	More lubrication; position changes	
During ejaculation	Long periods without sex; infection or swelling of the prostate gland	Continue to use System	Problem usually stops as you continue to use the system; if pain or discomfort continues, see your doctor
Redness, irritation or bruising	Too rapid pumping; overpumping	Slower pumping; fewer pumps	Consult your doctor if this problem continues past the first few practice sessions
Penis feels cold (to you or your partner)	Constriction of blood flow to the penis; lubrication	Wash off lubricant or warm lubricant before use	
Penis pivots on its base	Constriction of blood flow to the penis	If manageable, apply the system after you have a partial erection	

PRECAUTIONS

You will feel pressure while applying the vacuum. This is not harmful. If you feel discomfort, however, it may be a signal that you are pumping too quickly. Simply press the manual vacuum release button, wait a moment and start again.

Your penis turns slightly bluish in color after you apply the Erection Assistant Ring. This may be a normal response to the increase of blood in the penis. The bluish color should disappear when you remove the support ring.

You experience some petechiae (tiny reddish spots beneath the skin) or bruising of the penis when you first begin using your system. This may happen by placing the penis under to much vacuum pressure for too long, and too fast, or after a long period of not having an erection. If this happens, stop using your system until spots or bruises completely disappear, about five to seven days.

You or your partner notice a slight drop in the temperature of the penis. This coolness is normal and not harmful. It is a normal response to the reduced blood flow caused by the support ring.

Your erection has a "hinge" effect. The penis may pivot at its base when the ring is in place. If this occurs, you may find it necessary to try different positions with your partner for successful intercourse.

Your semen does not flow through at point of climax. The pressure of the Erection Assistant Ring may interfere with the ejaculation process. This is not harmful, and does not affect climax. Your semen may flow out when you remove the ring. Erection Assistant Rings are not a means of contraception or birth control and should not be used to avoid pregnancy.

Your penile Cylinder develops condensation on the inside. This is simply the result of the heat from your body reacting with the sealing gel. "Fogging" can be reduced by running warm water over the Cylinder and then drying it before use.

Use of  Vacuum Erection System may bruise or break the blood vessels either right below the surface of the skin or within the deep structures of the penis or scrotum, resulting in bleeding or the forming of a blood filled swelling. Do not be to concerned if you notice some bruising of the penis, or small reddish spots below the skin. This is likely to happen if you have not had sex for some time. You should stop using the system until the problem has cleared up (5 or 6 days). When you do use the system again, be careful not to apply more vacuum than feels comfortable. Use caution and plenty of water soluble sealing gel when removing the Erection Assistant Ring.

PRECAUTIONS

If you have signs of Erectile Dysfunction, (i.e., unable to get an erection that is strong enough for sexual intercourse), talk to your doctor before using this system to avoid a possible harmful delay in discovering any of the most common causes of this condition, such as diabetes, multiple sclerosis, cirrhosis of the liver, chronic renal failure, or alcoholism.

Do not wear the Erection Assistant Ring for longer than 30 minutes. It could cause pain, bruising, a blood blister, or permanent injury to the penis. Consult your doctor if any problems occur and stop using the system if they continue.

If you do not follow these instructions you may cause personal injury.



will not cure relationship problems or correct physical problems such as low sex drive, decreased sensation, and absent or premature ejaculation.

If you have Sickle Cell Trait or Disease, a history of prolonged erections, or are taking large quantities of aspirin or other blood thinners, do not use without consulting your doctor.

Misuse of or its Erection Assistant Rings may worsen already existing medical conditions such as Peyronie's Disease (a condition that causes distortion or abnormal bends of the erect penis), prolonged erection, and blocked urethra (urinary tract).

Misuse of or its Erection Assistant Rings could result in swelling of the penis or serious permanent injury to the penis.

Frequent use of the Erection Assistant Rings may result in bruising at the base of the penis (where the shaft of the penis meets the pubic area), blood blister or pain.



PRECAUTIONS



Expected patient age group 18+ adult, old age, contraindications

These devices should not be used with patients that have allergic to the specific material used. Moreover, instruments should not be used for anything other than their intended use.

shelf life/stability of the device

for 3 years from manufacturing date.

Maximum number of reuses of the  device 550-575 times.

ABS, (PC) Polycarbonate. PVC, Silicone, (medical grade).Packing Parachute bag.

The end of the device lifetime is usually determined by wear and damage from use. They are then to be disposed of according to local government procedure / regulatory requirements. Do not use any damaged device.

Limitation on reuse of device

The end of the device lifetime is usually determined by wear and damage from use. They are then to be disposed of according to local government procedure / regulatory requirements. Do not use any damaged device.

Storage:Store packaged device in dry place as per best practices to allow device to remain clean, dry, and ready for service.

Disposal:The device doesn't contain any toxic or hazardous material(s); when recycling medical devices please follow your local government Health & Safety procedures and regulatory requirements.

warranty:This product is guaranteed to be free from defects in material or workmanship. The warranty is null and void should product damage occur as a result of mis-handling or mis-use. Modifications carried out on devise may also result in loss of guarantee / warranty rights. Care must be taken in the use handling and use of this product."

Return:In case of damage or faulty, please return to supplier with same packaging and event description.

Note: after the return receiving  immediately destroy



PRECAUTIONS

It helps boost blood flow to the penis, triggering an erection within minutes,

Not recommended for erectile dysfunction Testosterone.
It's a male hormone. If you have normal testosterone level,
you don't need more



Instructions/warnings.

Never attempt to make repairs yourself. Any repairs made by the users may void the warranty.

Never store damp instruments. They must be thoroughly dried first.

Always ensure device is only used for the purpose for which they were designed.

Always handle all device gently. Never overstrain, drop or misuse them.

Always periodically check the condition of the device. Discard the damaged device.

Always check all device for damage before and after use.

Prior to use, visually inspect the instrument for bent, broken, cracked, worn, or missing component(s).

Do not use the device if it is damaged or defective.

Always ensure devices are thoroughly dried before being stored.

Always use the devices on doctor's prescription.

Always follow recommended local government Health & Safety procedures and regulatory requirements.

Always follow recommended procedure for cleaning.

Inspect device for good cleaning result and repeat procedure if necessary.

The best effects are achieved by cleaning the device immediately after each application.

Always properly cover the clean device before storage.



 Europe No. RPS/68/2021-CMC

By:

AMFAH INTERNATIONAL



3/416-19B, Pasrur Road, St#4,

Daska 51010 (Distt), Sialkot Pakistan

Email ID: info@Erect-D.com

www.Erect-D.com